




Phonak Virto M-10 NW O (M90/M70/M50/M30)

M Receiver


2 cm³ coupler data

ANSI / ASA S3.22-2014
IEC 60118-0 : 2015

Output sound pressure level

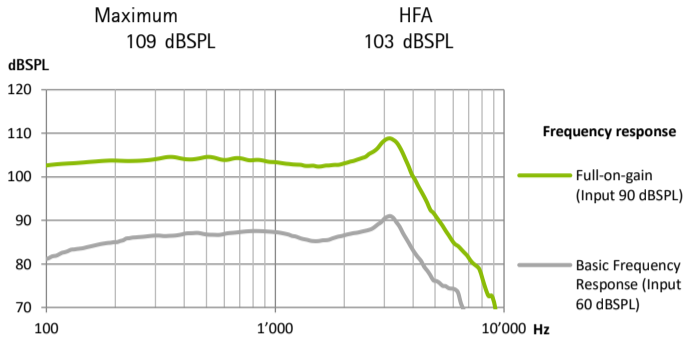


Acoustic gain

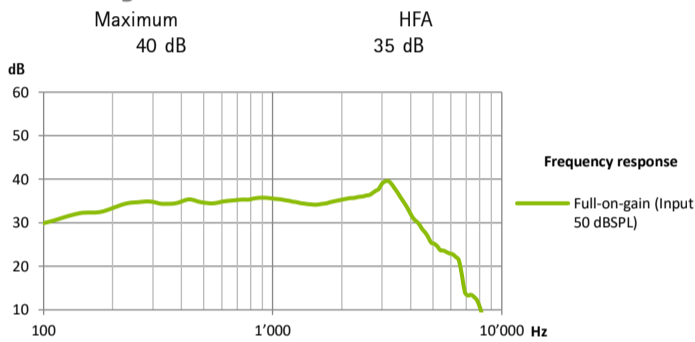

Frequency range	<100 Hz - 7000 Hz			
Total harmonic distortion	500 Hz	800 Hz	1600 Hz	3200 Hz
	1.0%	1.5%	1.0%	1.0%
Battery current	1.0 mA			
Equivalent input noise level	19 dB SPL			

Induction coil sensitivity

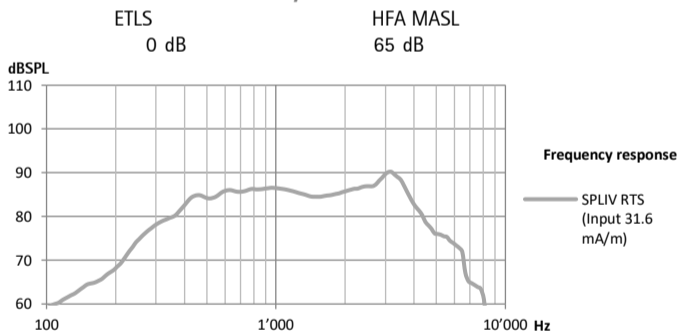


P Receiver


2 cm³ coupler data

ANSI / ASA S3.22-2014
IEC 60118-0 : 2015

Output sound pressure level

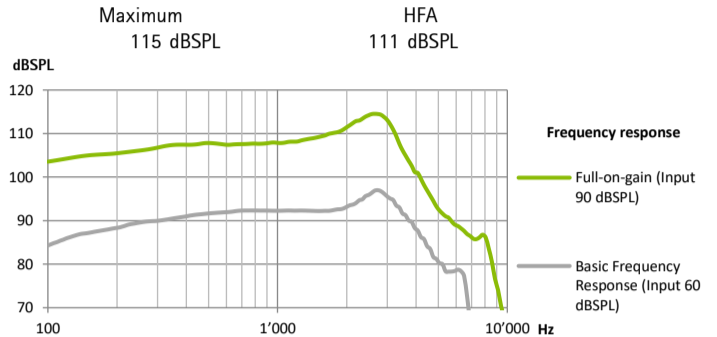


Acoustic gain

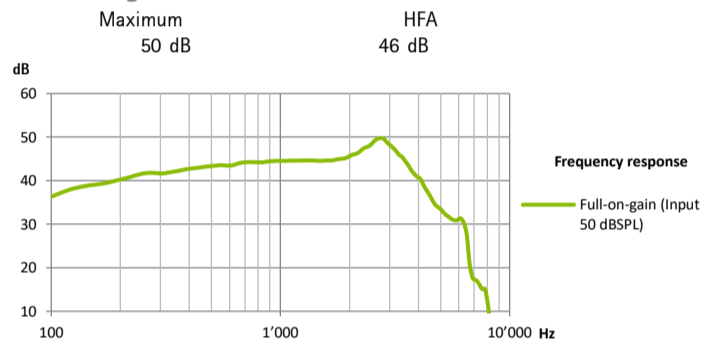

Frequency range	<100 Hz - 6700 Hz			
Total harmonic distortion	500 Hz	800 Hz	1600 Hz	3200 Hz
	1.0%	1.0%	1.0%	1.0%
Battery current	1.0 mA			
Equivalent input noise level	19 dB SPL			

Induction coil sensitivity

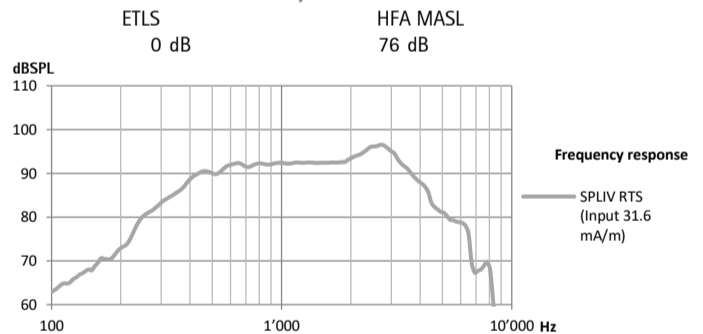

General test information

- Supply voltage 1.3 V / impedance 6.2 Ω
- Specific measurement settings are used. RTS adjustment with volume control
- The device is operating in linear mode
- Low-level expansion is active
- Unless otherwise specified, all data obtained are measured with 5 mm tubing and Phonak Target measurement settings

⚠ WARNING: Changes or modifications to the hearing aid that are not explicitly approved by the manufacturer are not permitted. Such changes may damage the ear or the hearing aid




Phonak Virto M-10 NW O (M90/M70/M50/M30)

SP Receiver


2 cm³ coupler data

ANSI / ASA S3.22-2014
IEC 60118-0 : 2015

Output sound pressure level

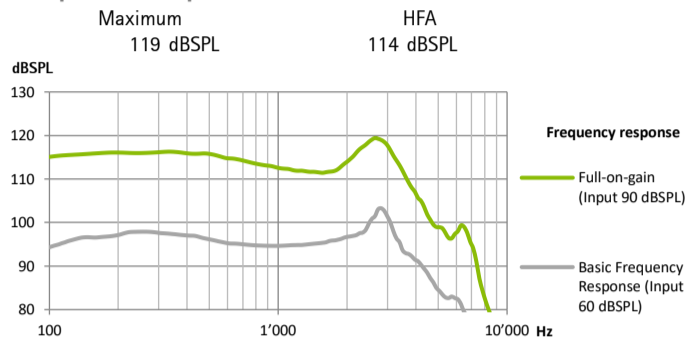


Acoustic gain

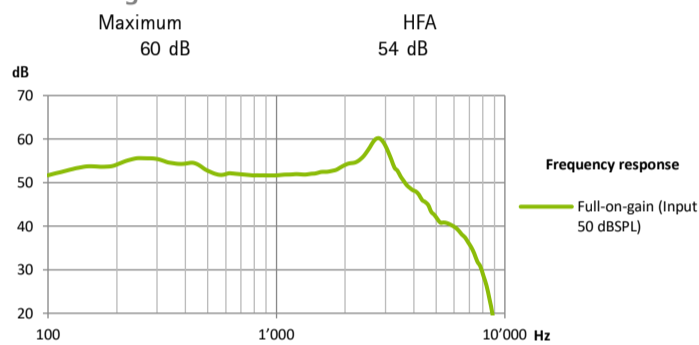

Frequency range	<100 Hz - 7000 Hz			
Total harmonic distortion	500 Hz	800 Hz	1600 Hz	3200 Hz
	1.0%	1.0%	1.0%	1.0%
Battery current	1.0 mA			
Equivalent input noise level	19 dBSPL			

Induction coil sensitivity

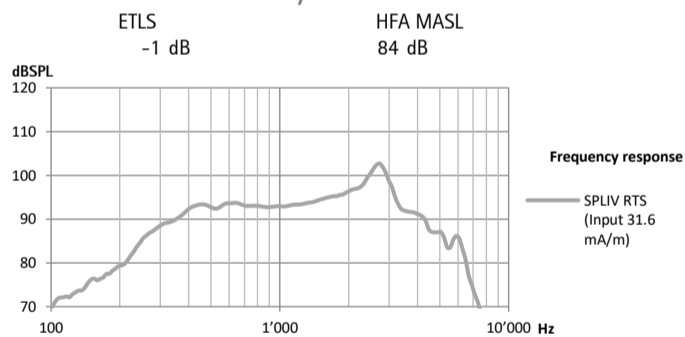

Absolute Hearing Solutions LLC

absolutehearing@att.net

750 Cross Pointe Road Suite F
Gahanna, Ohio 43230

Phone: 614-452-4260
Toll Free: 888-803-2159
Fax: 614-577-0461

www.absolutehearing.com



Sonova AG · Laubisrütistrasse 28
CH-8712 Stäfa · Switzerland
www.phonak.com

A Sonova brand

PHONAK
life is on